


PAJUNK®



NerveGuard

*Automatic Injection
Pressure Limiter*

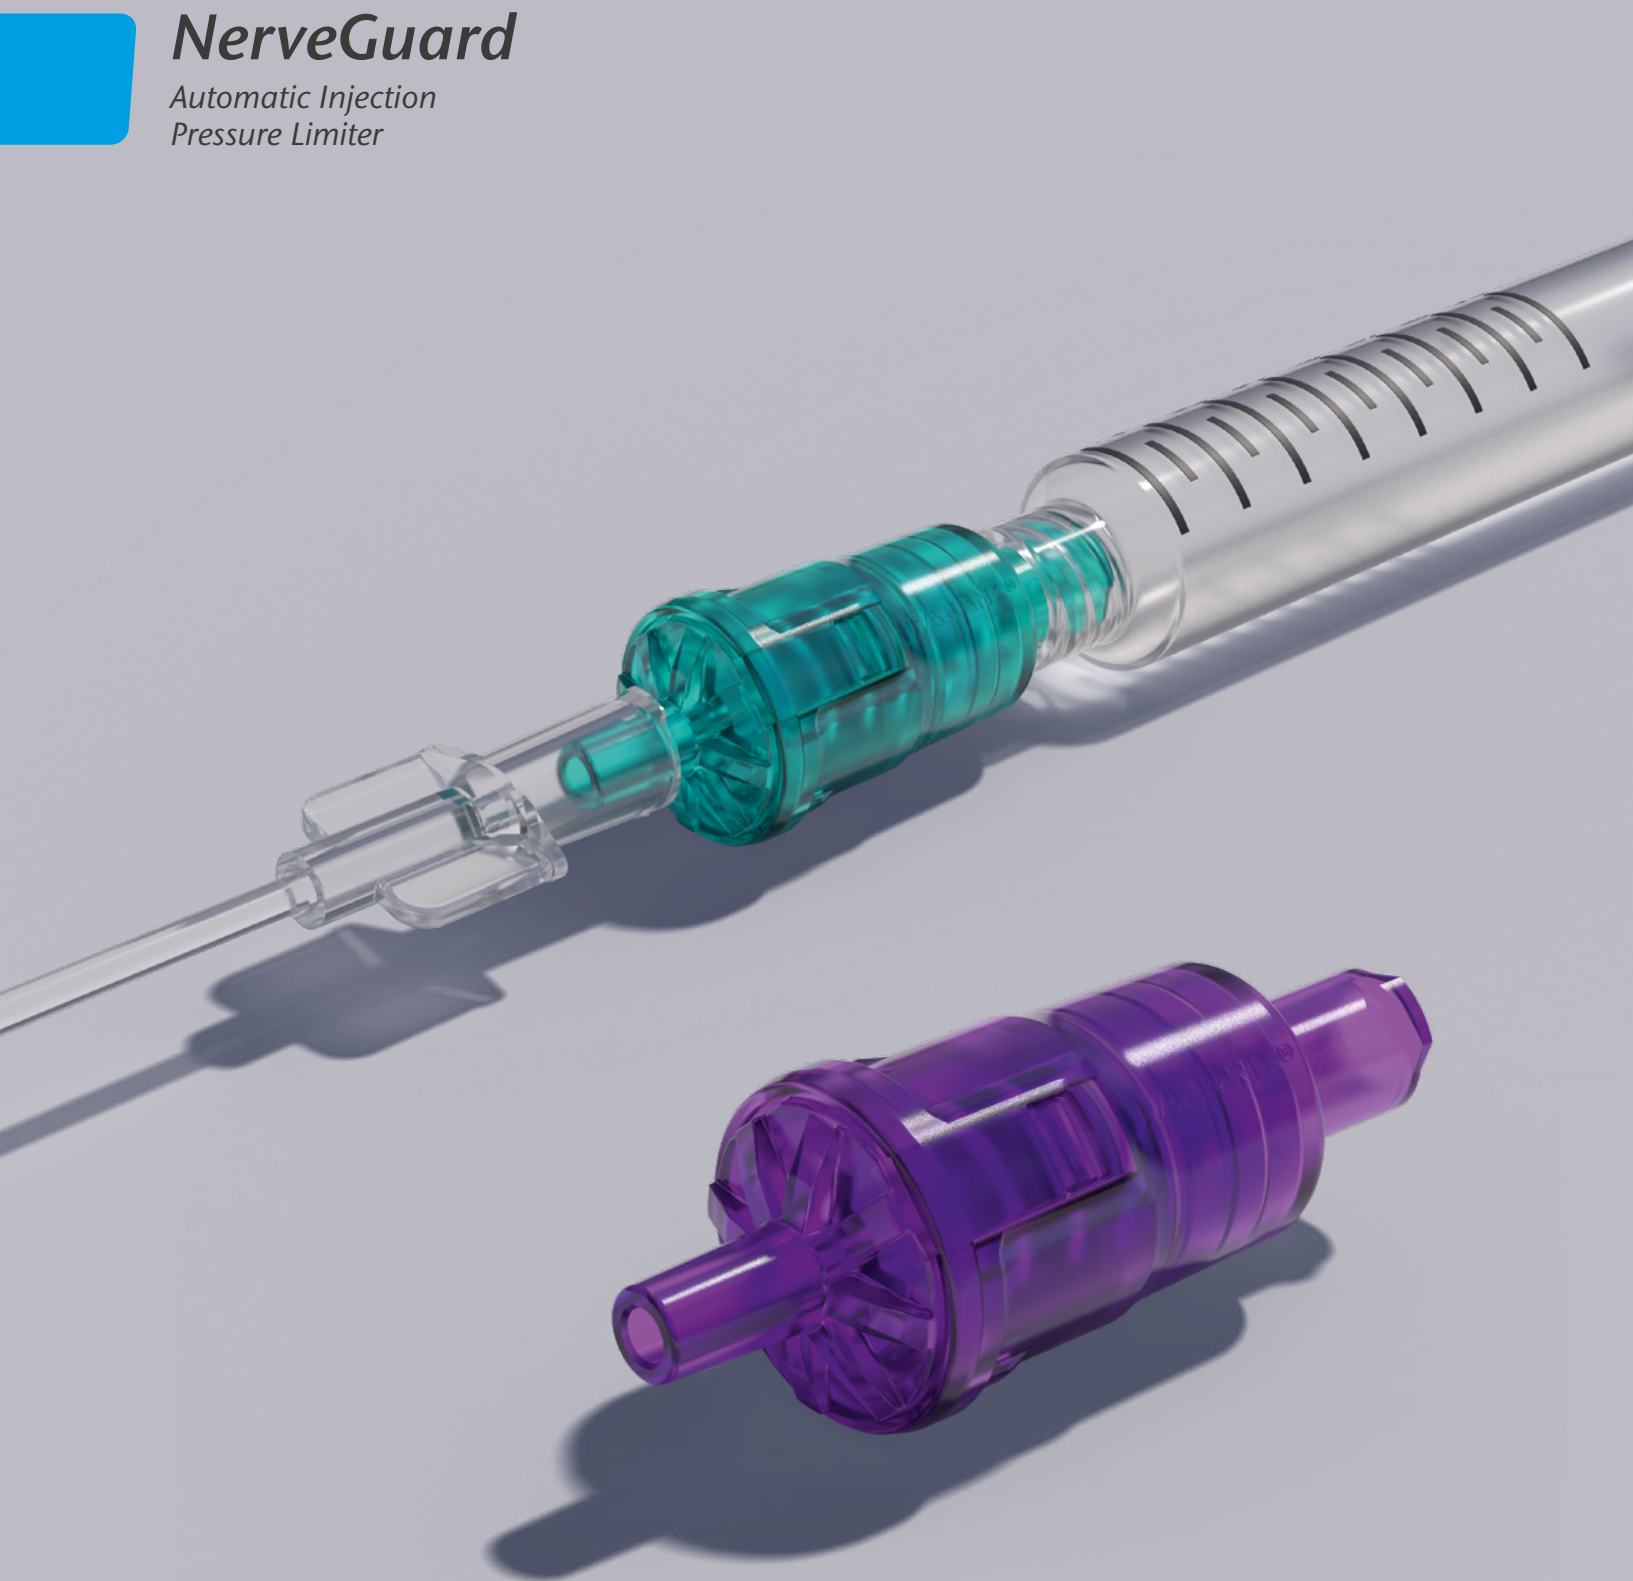

NerveGuard

The Automatic Injection Pressure Limiter



Also available in **NRFit**

Ultrasound-guided localisation of peripheral nerves and the associated real-time visualisation provide crucial benefits in regional anaesthesia.¹ Nonetheless, it is clear that this does not reduce the incidence of permanent nerve damage.² Even in combination with nerve stimulation, intrafascicular injections cannot be ruled out.^{1,3,4,5} The causes include incorrect positioning of the needle along with exceeding critical injection pressures. With the NerveGuard, developed by Pajunk, the injection pressure is automatically limited to avoid nerve damage.



For **single shot** applications
in diameters of
20G / 21G / 22G

For **single shot** applications
in diameters of
24G / 25G



HOW IT WORKS

- ▶ Automatically blocks injections when injection pressure exceeds the limit value
- ▶ No monitoring and no visual control necessary

- Detects incorrect needle positioning (fascia or nerve contact)
- Prevents intrafascicular injections in cases of excessive pressure
- Provides important information regarding position correction
- Avoids nerve damage and increases patient safety

1. Choquet O., Capdevila X. Ultrasound-guided nerve blocks: the real position of the needle should be defined. *Anaesth. Analg.* 2012 May; 114(5): 929-930
2. Neil J. M., Brill R., Horn J. L., Liu S. S., McCartney C. J., Perlas A., Salinas F. V., Tsui B. C. The Second American Society of Regional Anesthesia and Pain Medicine Evidence-Based Medicine Assessment of Ultrasound-Guided Regional Anesthesia. *Reg. Anaesth. Pain Med.* 2016 March-April; 41(2): 181-194
3. Robards C., Hadzic A., Somasundaram L., Iwata T., Gadsden J., Xu D., Sala-Blanch X. Intrafascicular injection with low-current stimulation during popliteal sciatic nerve block. *Anesth.* 2009 Aug; 109(2): 673-677
4. Vassiliou T., Müller H. H., Limberg S., De Andres J., Steinfeldt T., Wiesmann T. Risk evaluation for needle-nerve contact related to electrical nerve stimulation in a porcine model. *Acta Anaesth. Scand.* 2016 Mar; 60(3): 400-406

Description	Item no.	Item no. NRFit®	PU
NerveGuard / single / sterile / For single shot applications in diameters of 22G / 21G / 22G	001151-38M	001163-38M	10
NerveGuard / single / sterile / For single shot applications in diameters of 24G / 25G	001151-38N	001163-38N	10

PAJUNK® GmbH Medizintechnologie
Global Headquarters
Karl-Hall-Straße 1
78187 Geisingen, Germany
Tel.: +49 7704 9291-0
Fax: +49 7704 9291-600
info@pajunk.com
pajunk.com

PAJUNK® Medical Produkte GmbH
Central Europe
Karl-Hall-Straße 1
78187 Geisingen, Germany
Tel.: +49 7704 8008-0
Fax: +49 7704 8008-150
info@pajunk-medipro.com
pajunk.com

PAJUNK® Medical System L.P.
United States of America
4575 Marconi Drive
Alpharetta, GA 30005, USA
Tel.: +1 888 972 5865
Fax: +1 678 514 3388
info@pajunk-usa.com
pajunkusa.com

PAJUNK® UK Medical Products Ltd
United Kingdom
Unit D1 The Waterfront
Goldcrest Way, Newburn Riverside
Newcastle upon Tyne, NE15 8NY, UK
Tel.: +44 191 264 7333
info@pajunk.co.uk
pajunk.co.uk